




# FDA TEST RESULTS

**FDA Approval of the Odorox<sup>®</sup> MDU/Rx<sup>™</sup>  
Device for Use in Medical Facilities**

HGI INDUSTRIES INC.


# A. Niger - Reduction in Viable Concentration vs. Time

Control + Triplicate MDU Decon Runs, Collison Nebulizer, AGI-30 Impinger Enumeration

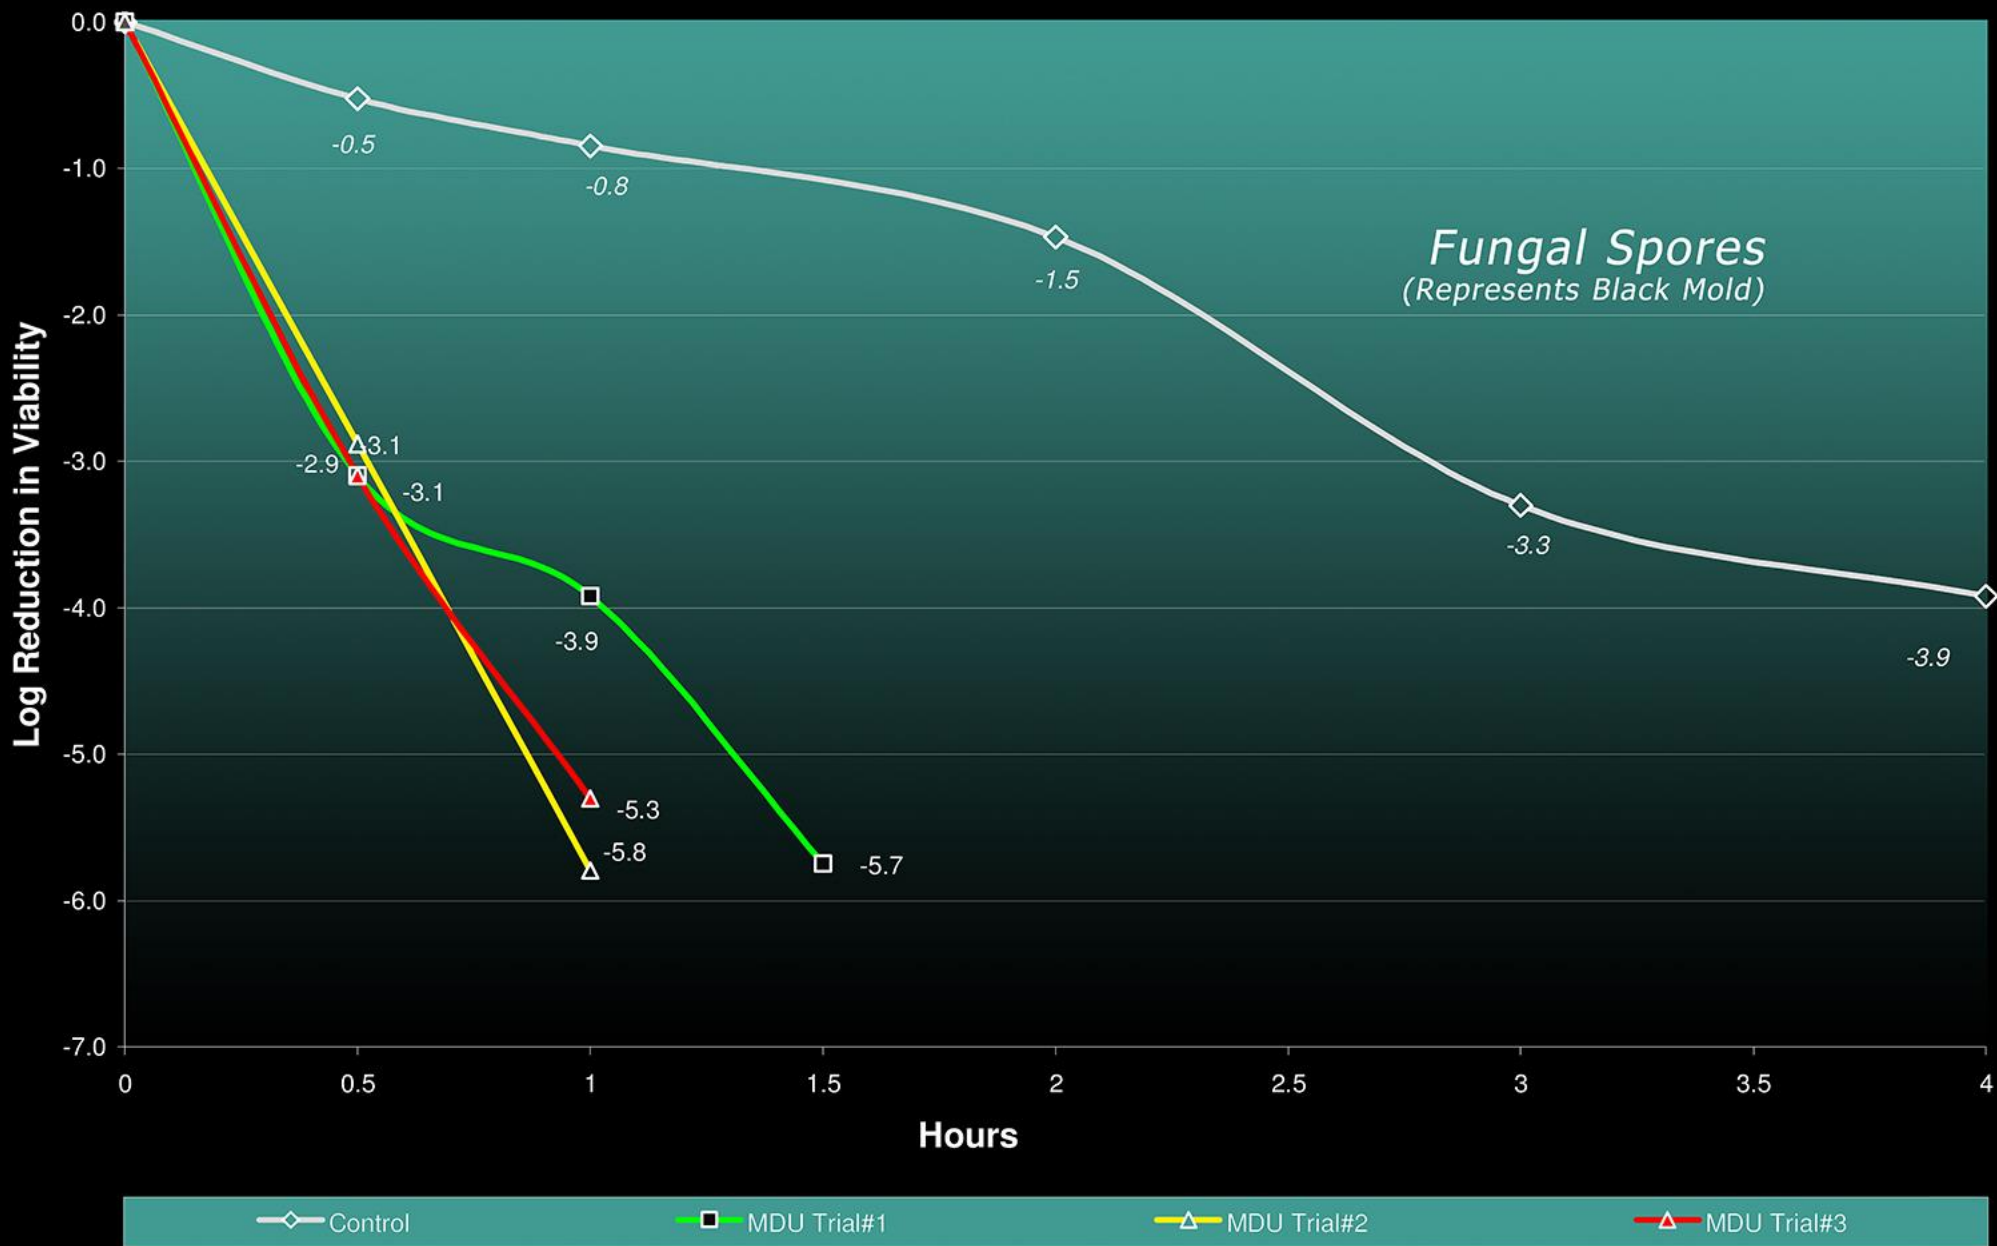


# *E. herbicola* - Reduction in Viable Concentration vs. Time

Control + Triplicate MDU Decon Runs, Collison Nebulizer, AGI-30 Impinger Enumeration

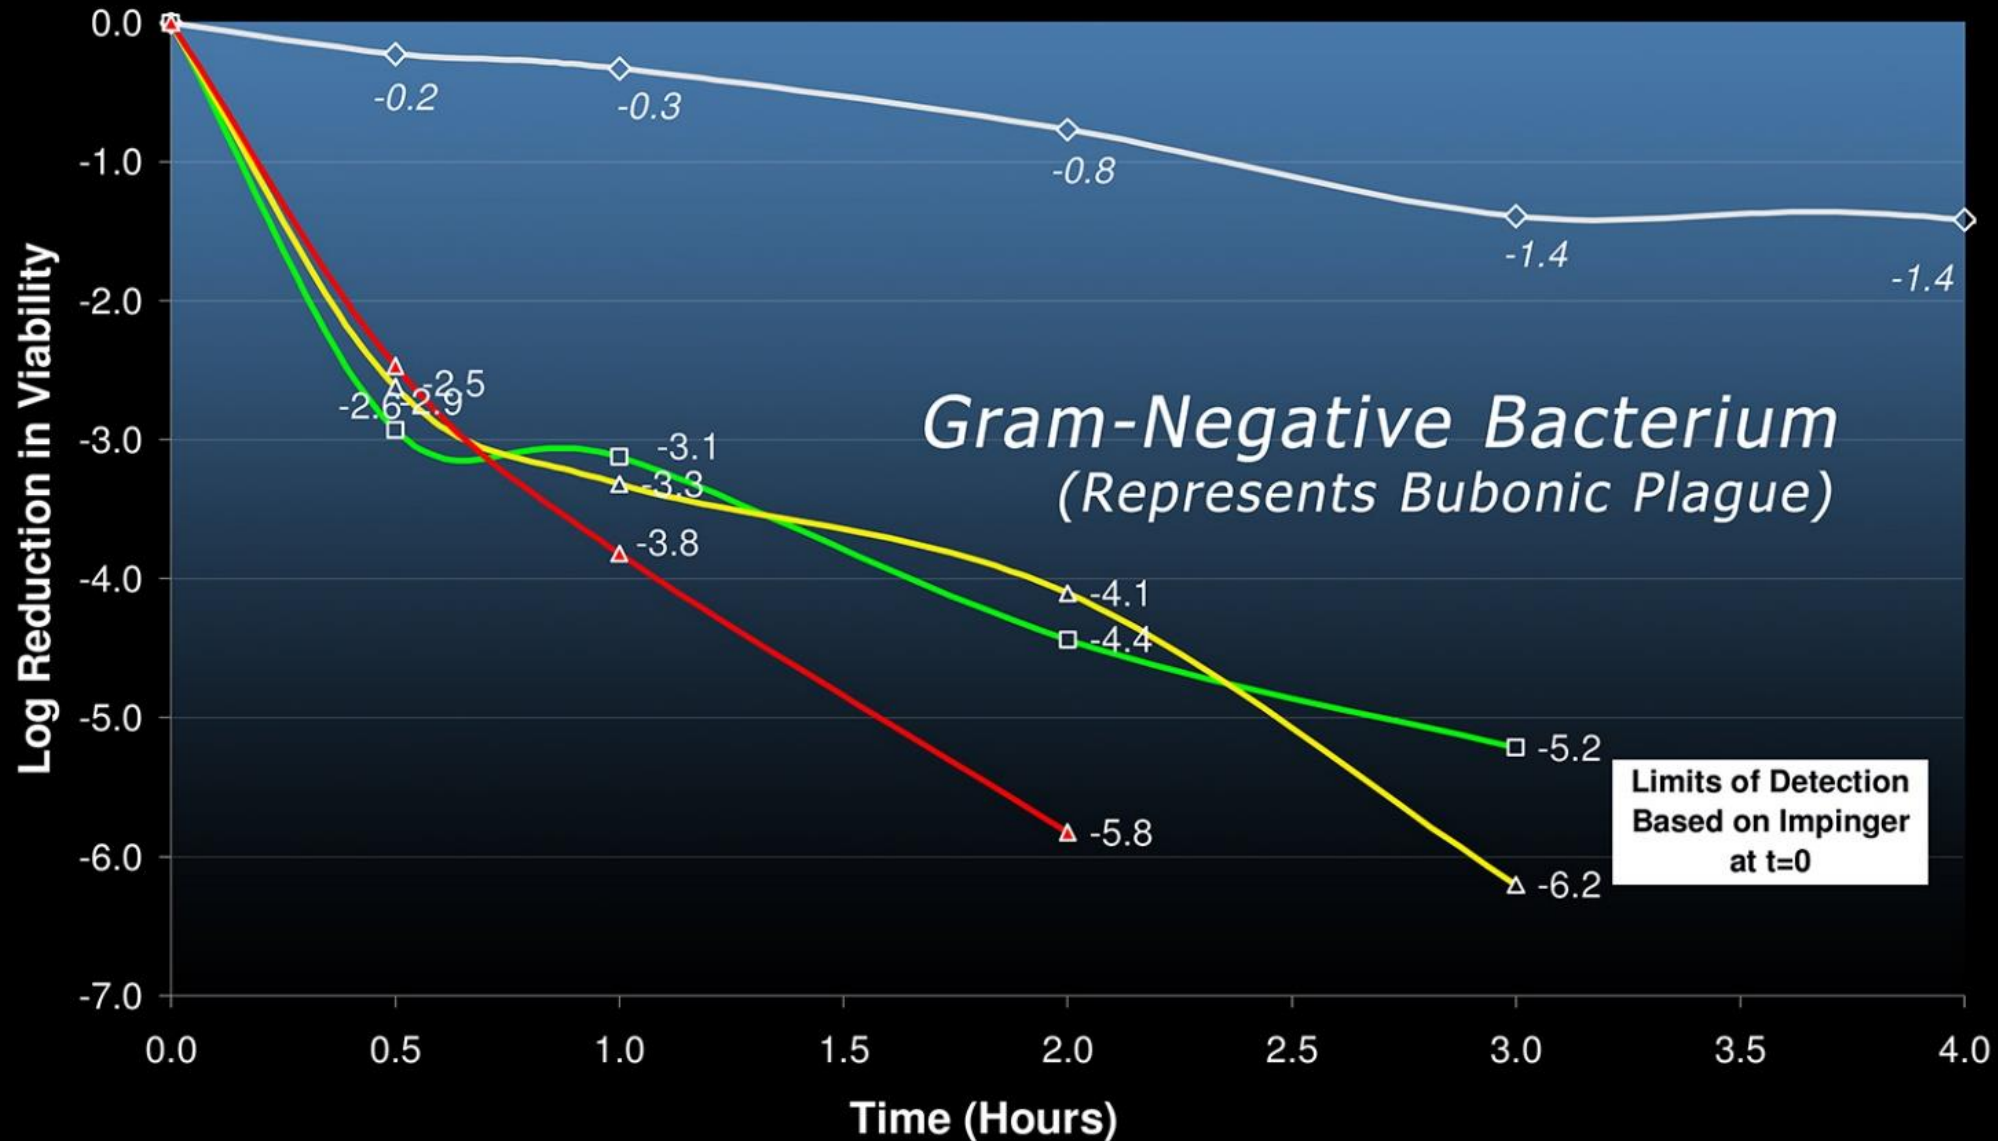

# MS2 - Reduction in Viable Concentration vs. Time

*Control + Triplicate MDU Decon Runs, Collison Nebulizer, AGI-30 Impinger Enumeration*

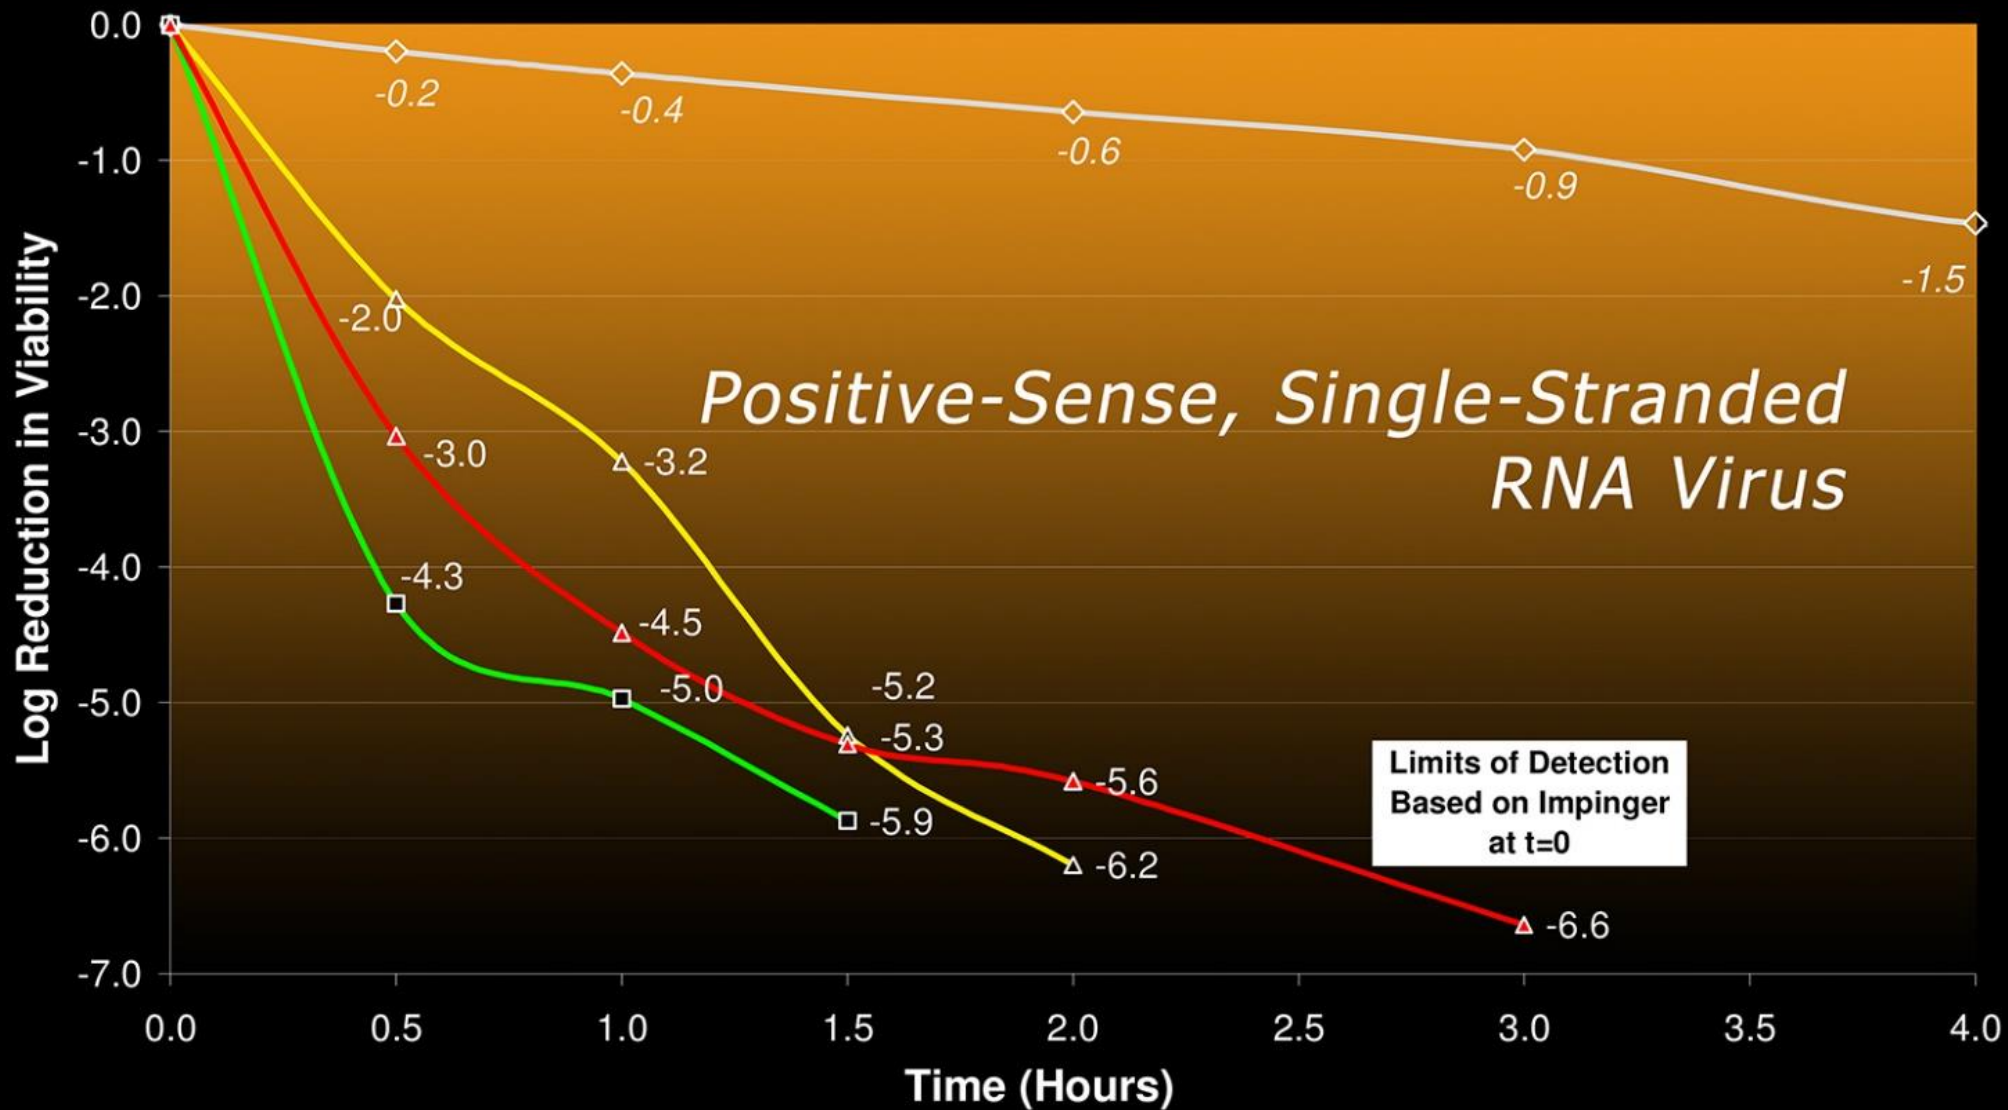

◇ Control


■ MDU Trial#1

△ MDU Trial#2

△ MDU Trial#3

# PhiX174 - Reduction in Viable Concentration vs. Time


Control + Triplicate MDU Decon Runs, Collison Nebulizer, AGI-30 Impinger Enumeration

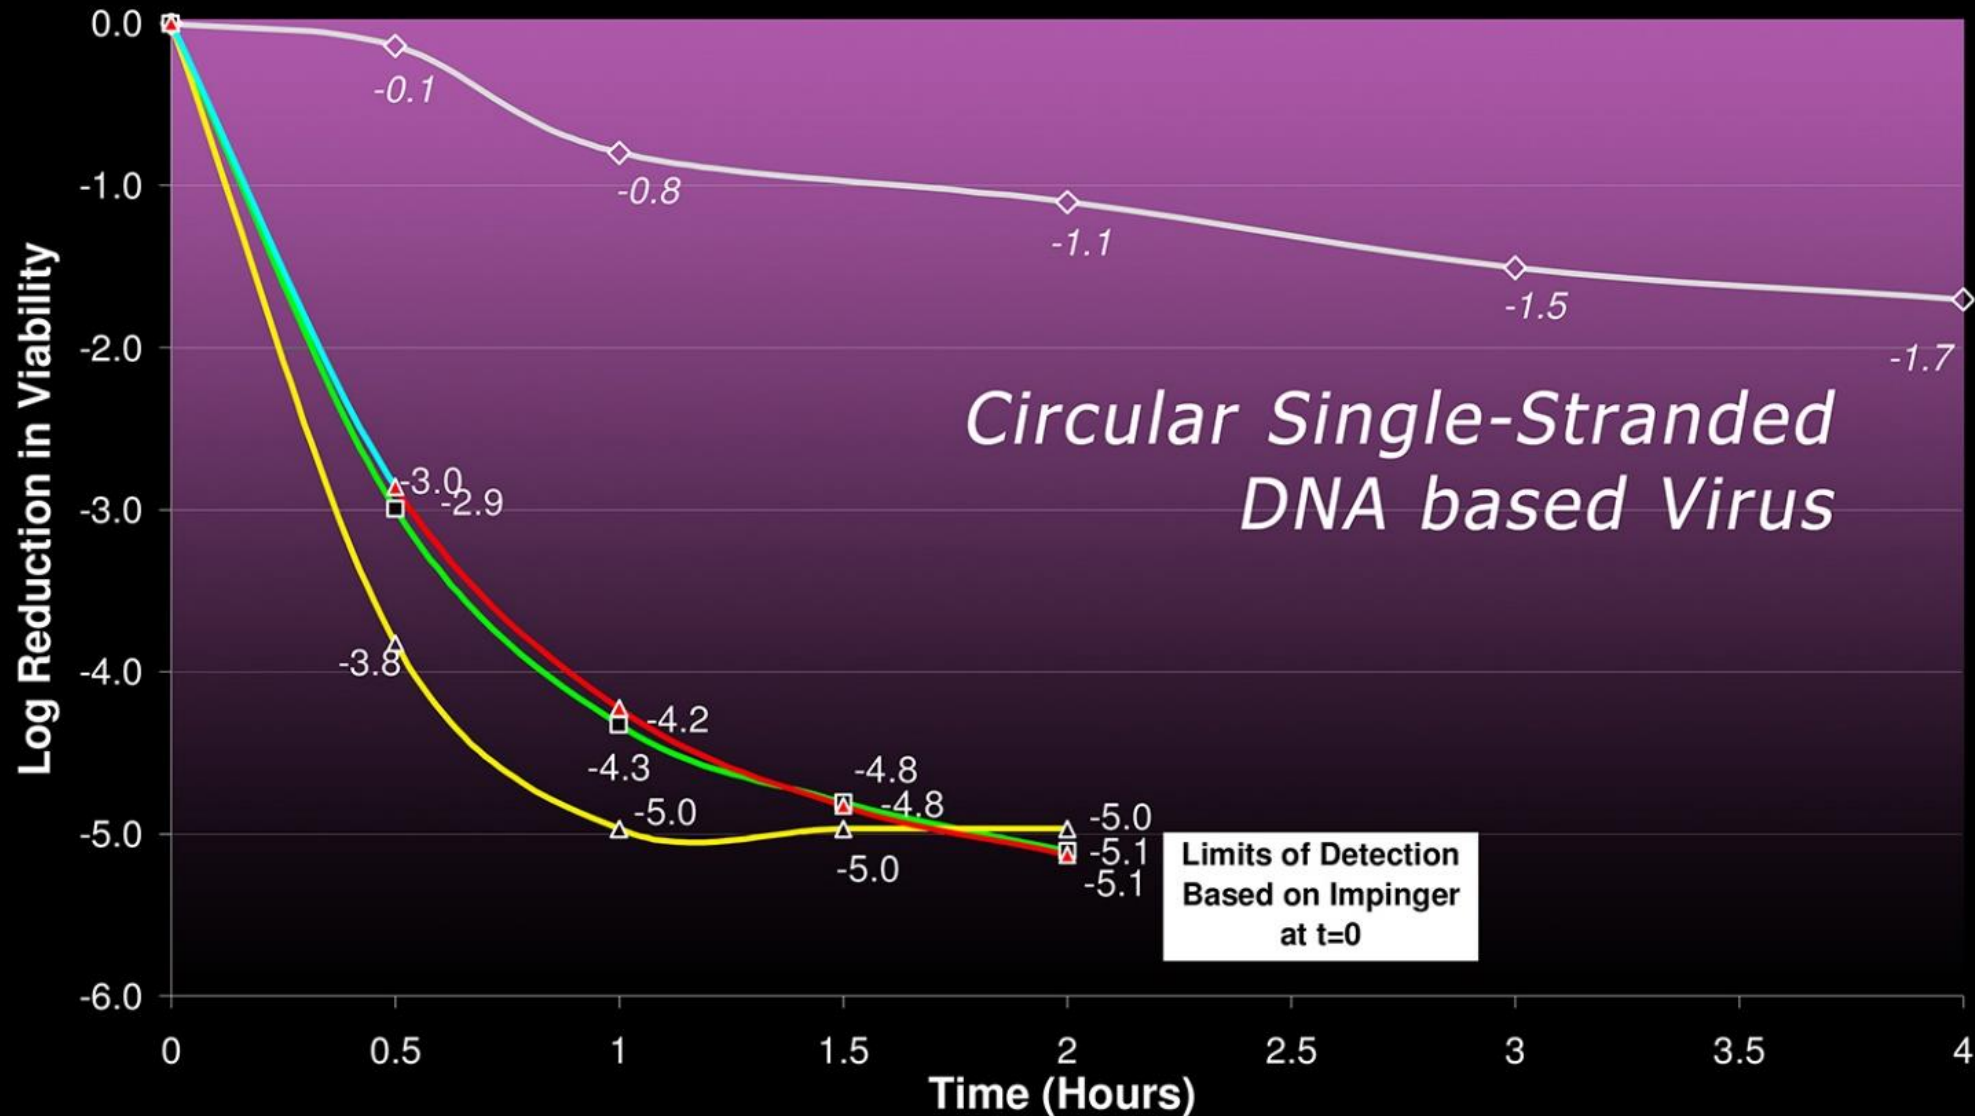



# Staphylococcus epidermidis - Reduction in Viable Concentration vs. Time

*Control + Triplicate MDU Decon Runs, Collison Nebulizer, AGI-30 Impinger Enumeration in Triplicate*

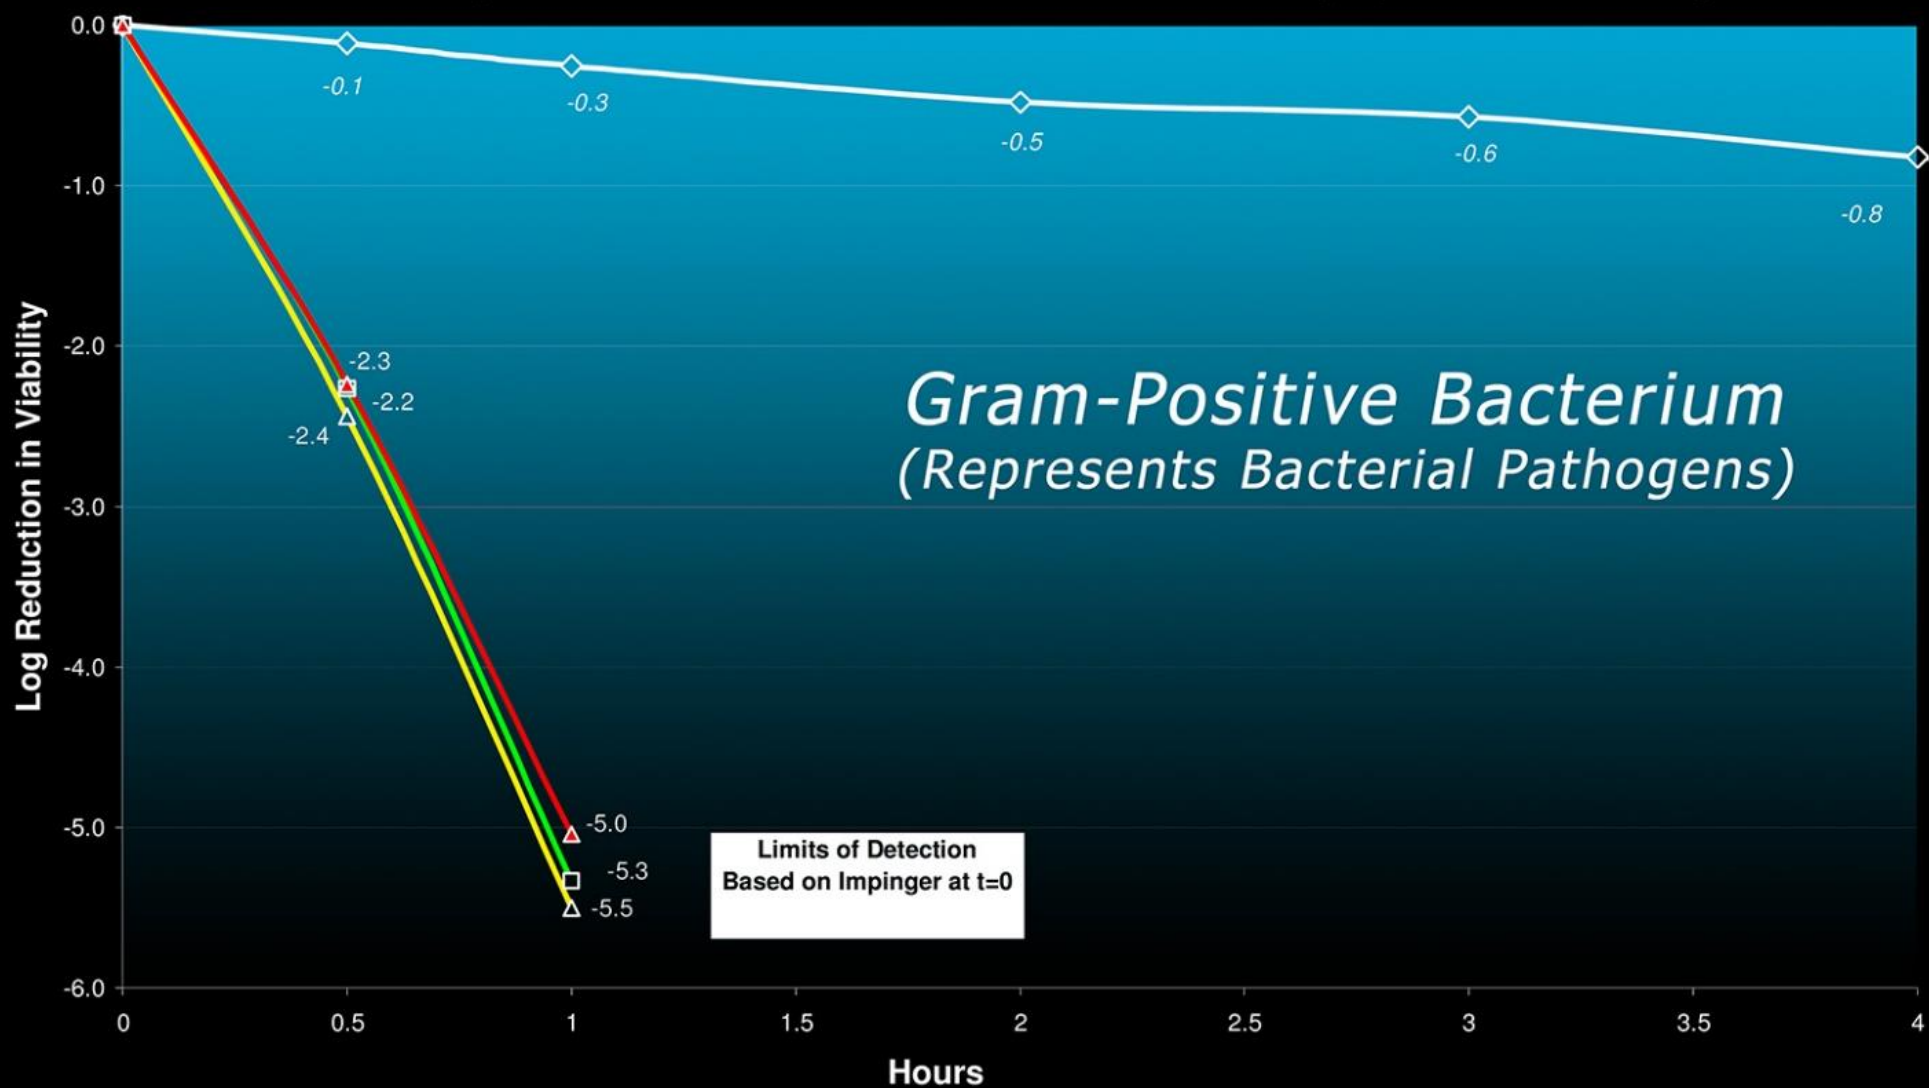

# Summary MDU/Rx™ Log Reduction Over Control

*Large Chamber, Average +/- ST. Dev Log Reduction, Triplicate MDU/Rx Trials*

